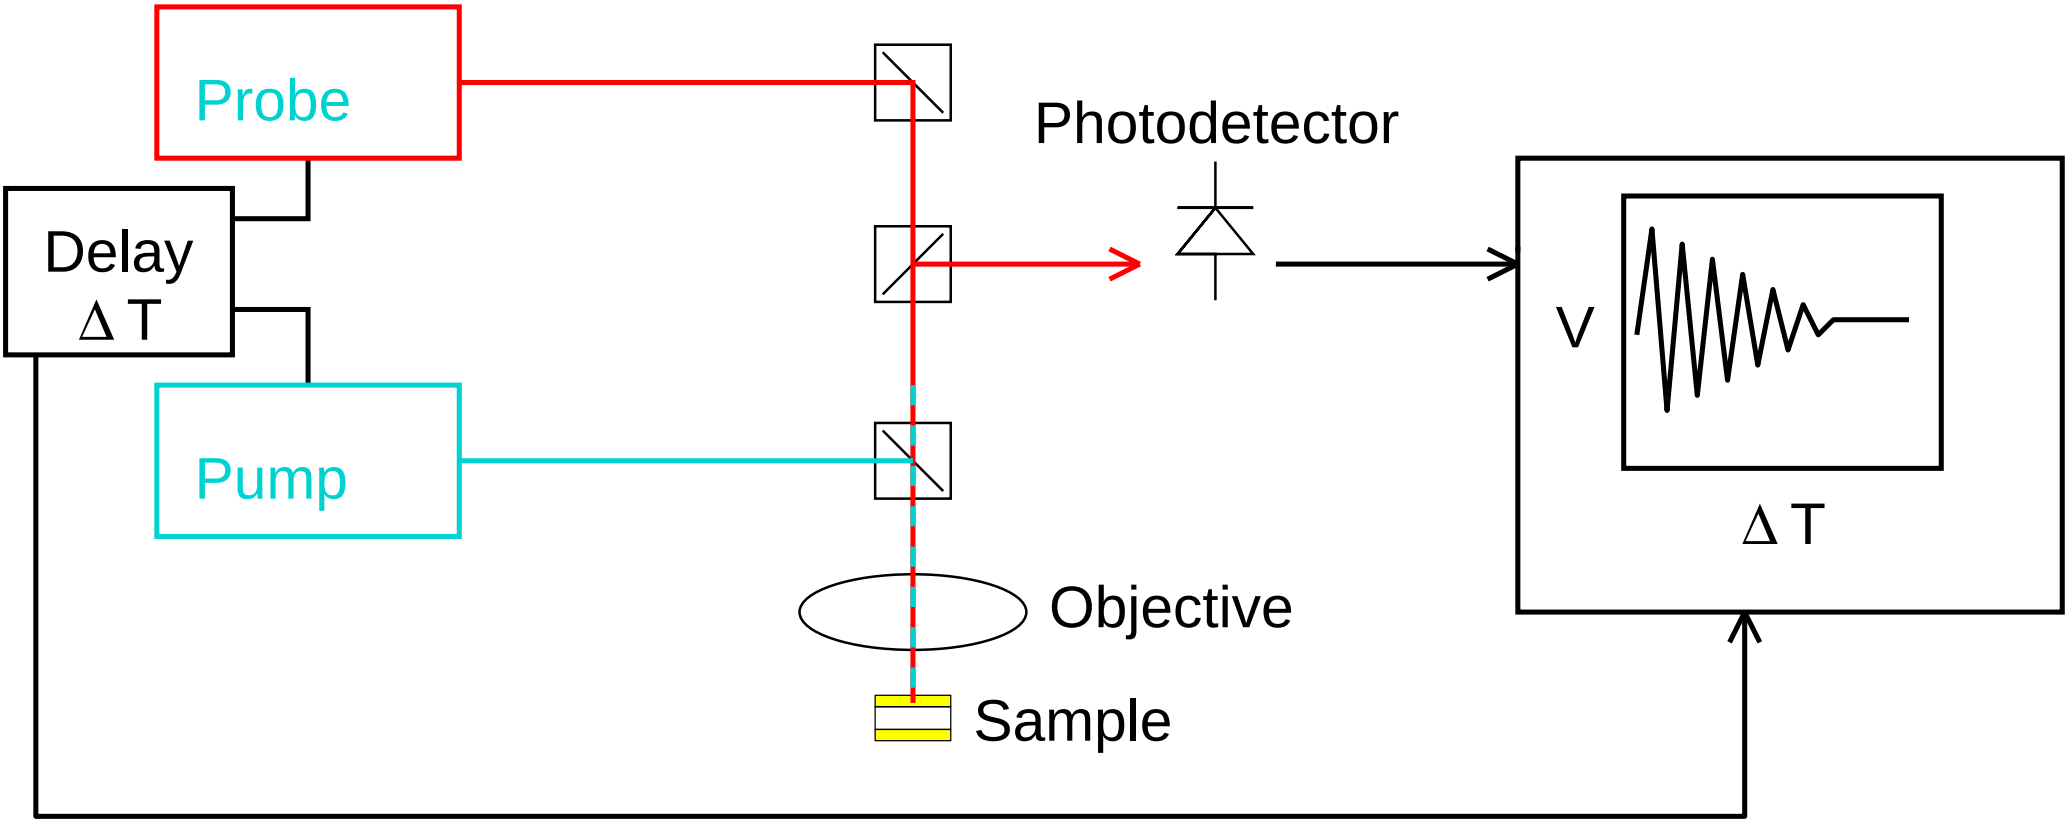
Probe
Delay
Δ T
Pump
Photodetector
V
Δ T
Objective
Sample